

FIG. 2C



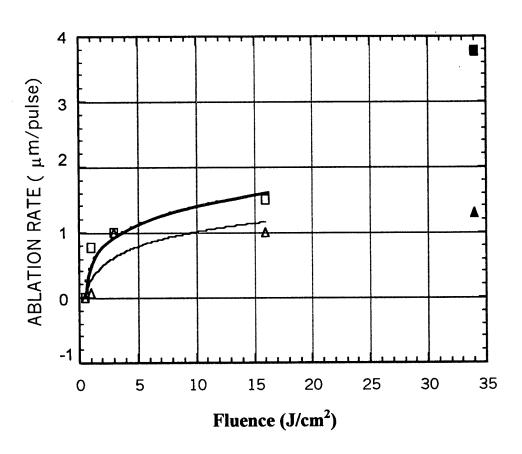


FIG. 3A





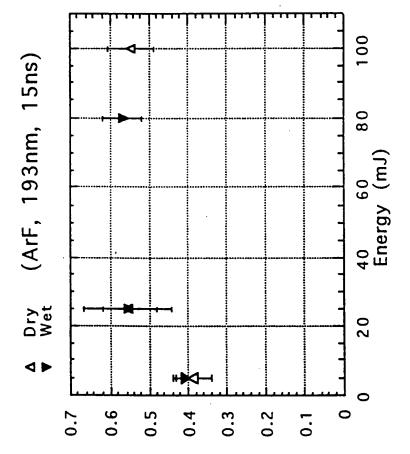

Ablation Rate (µm/pulse)

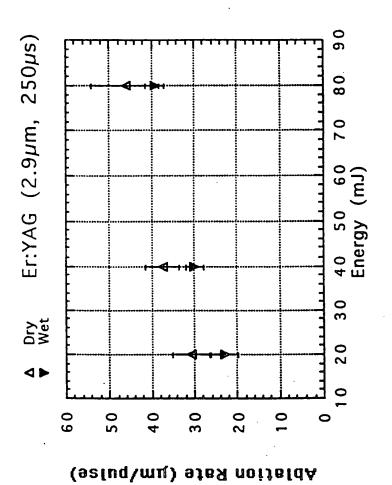


FIG. 3c

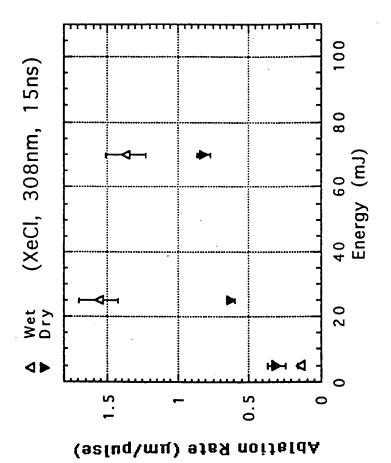


FIG. 3d

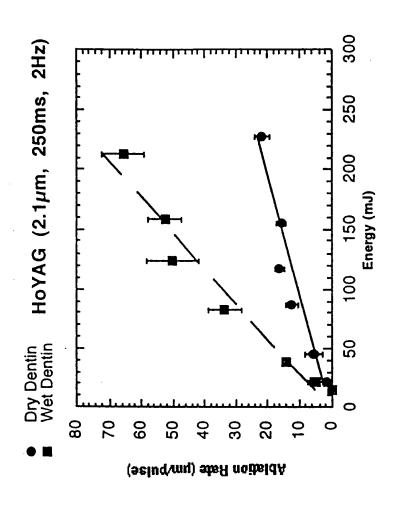


FIG. 36

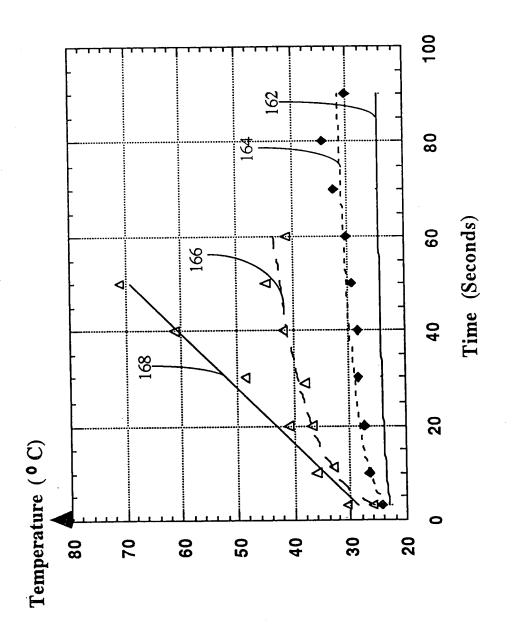


Fig. 4a

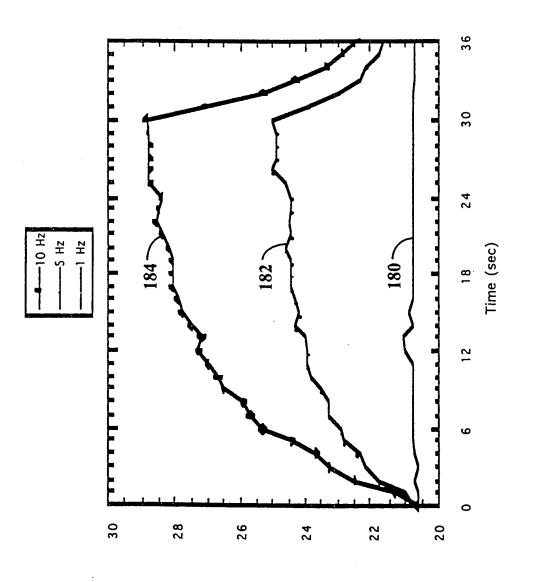
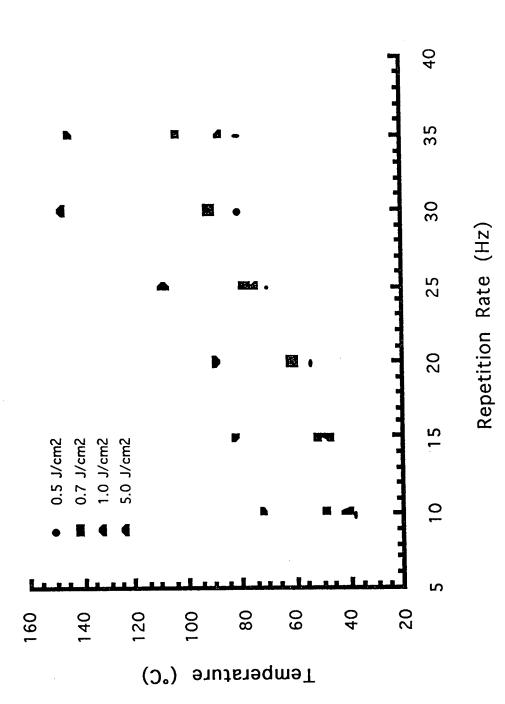


FIG. 4b

Temperature (⁰ C)



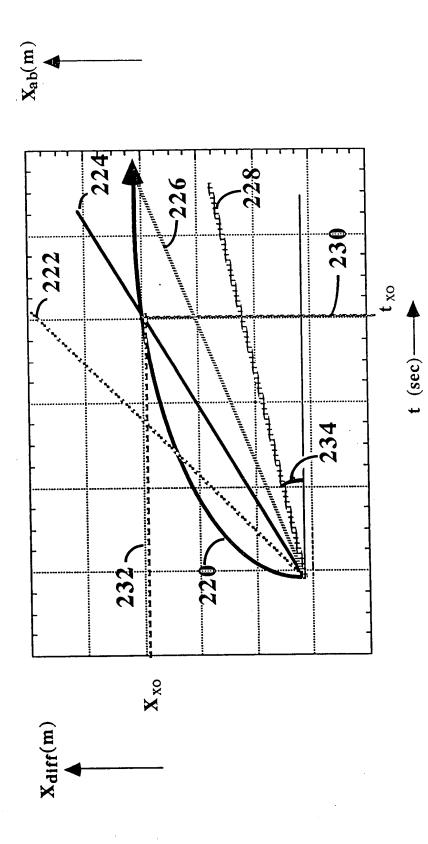
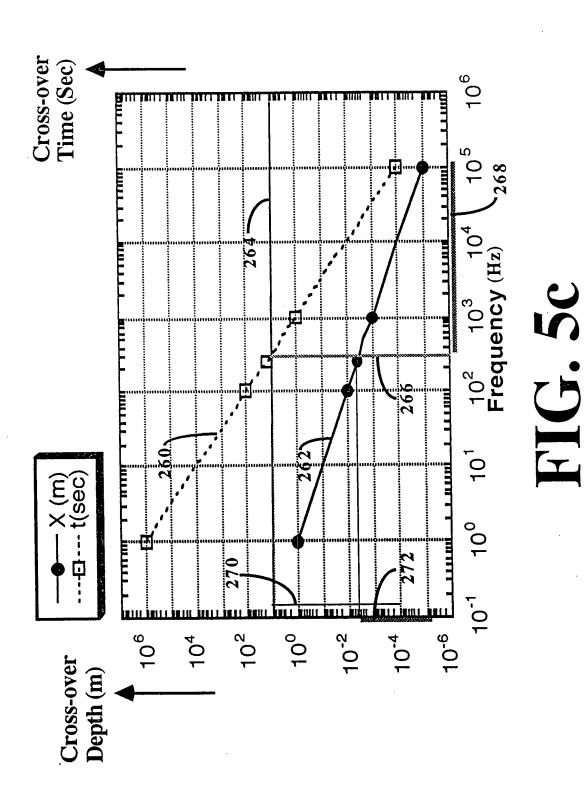


FIG. 5a

dozoso ostatec



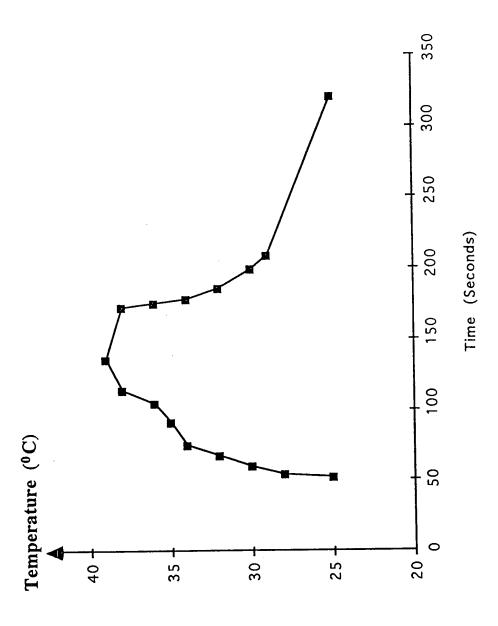


Fig. 5d

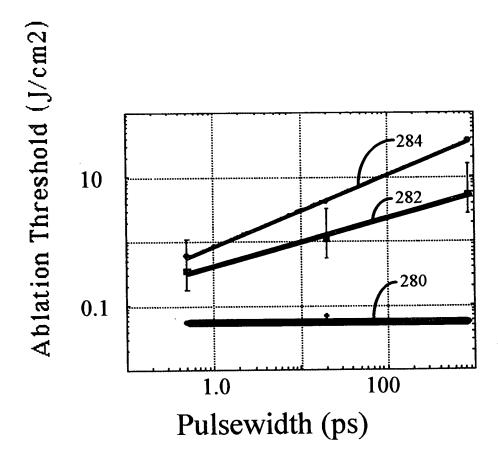
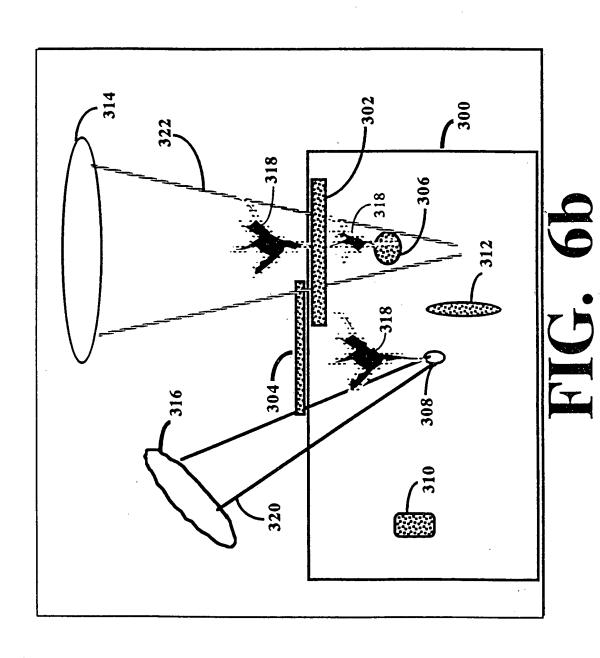
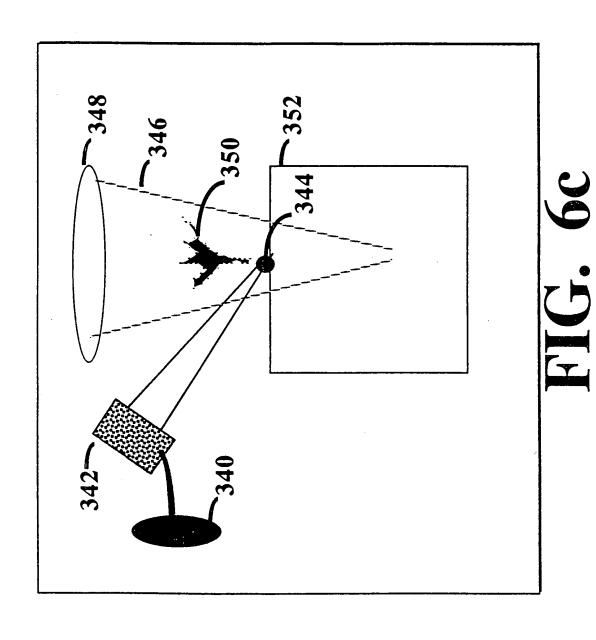


FIG. 6A





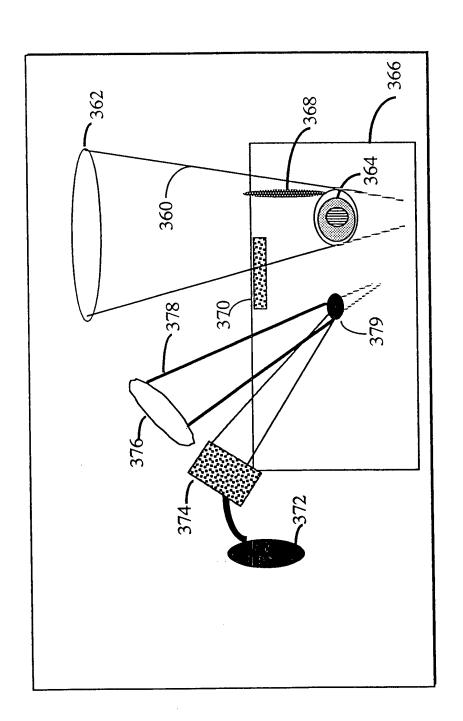


FIG. 7

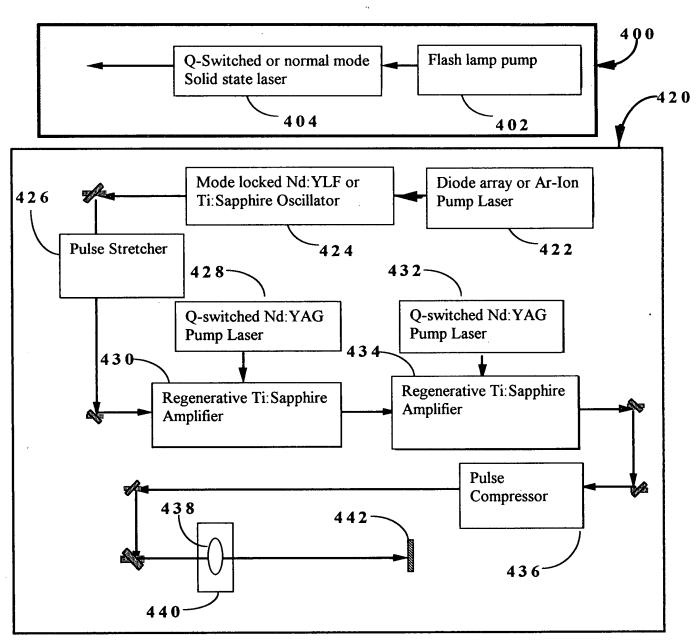


Fig. 8a

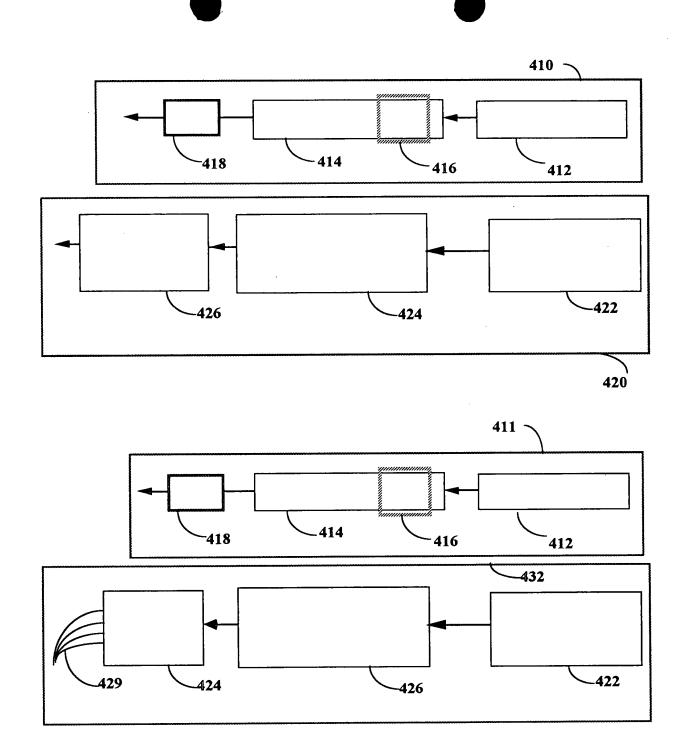
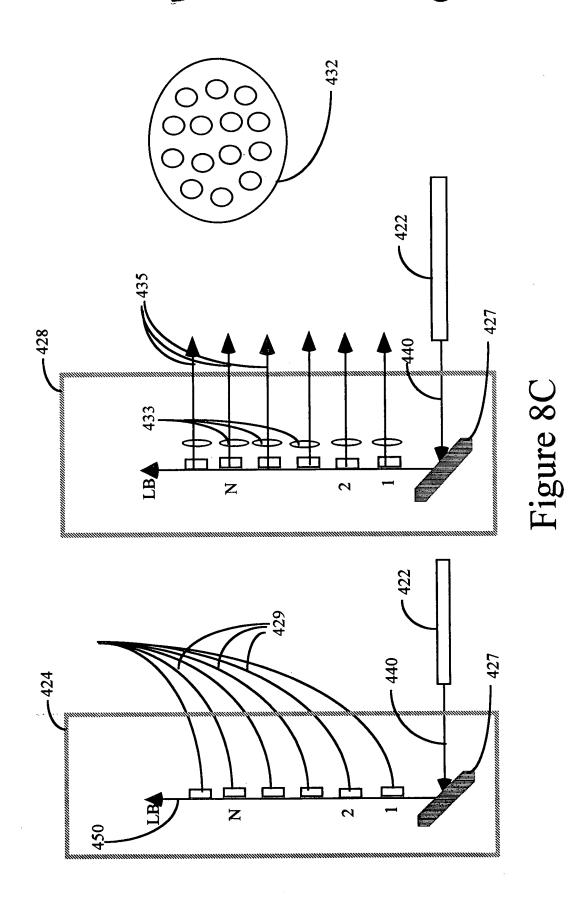
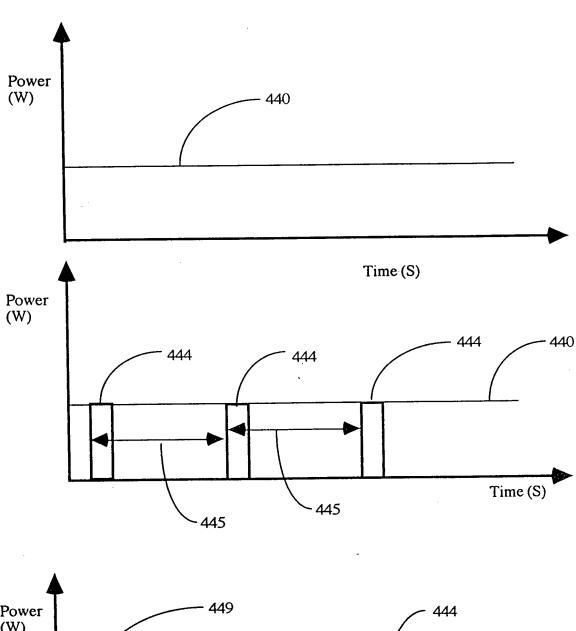


Fig. 8B





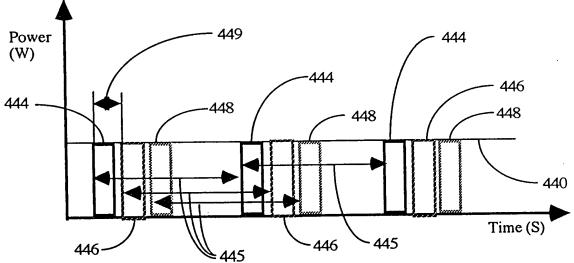
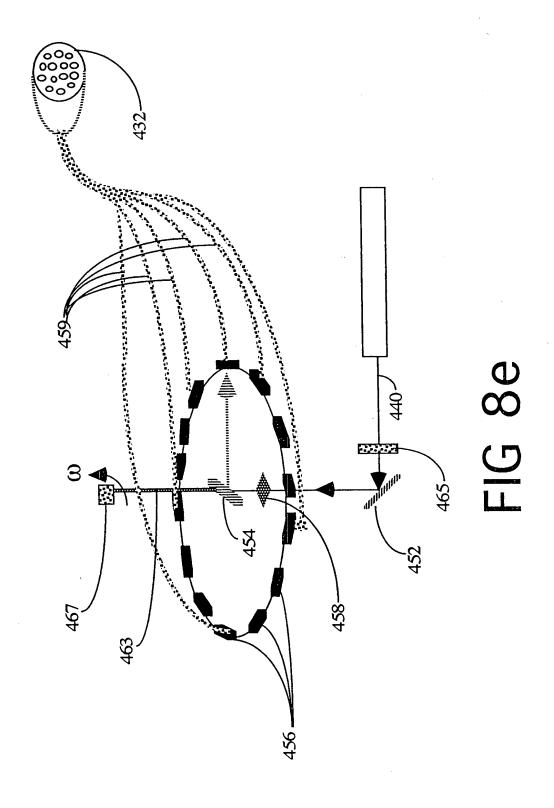


Fig. 8d



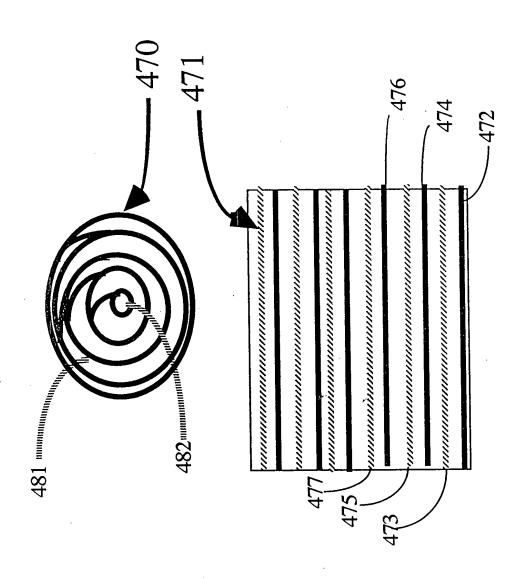
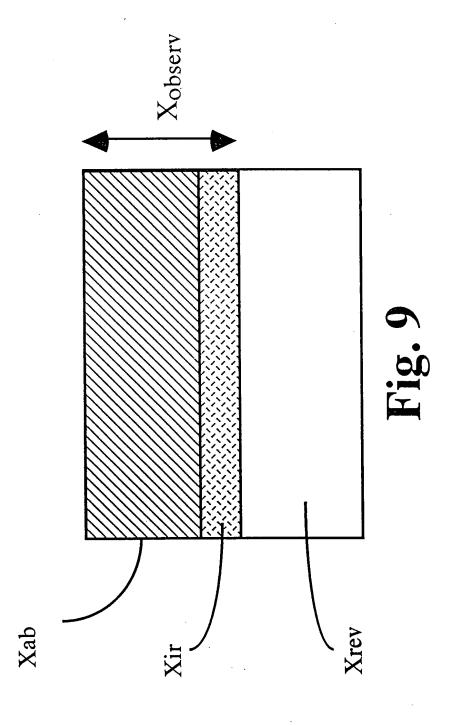


FIG. 8f

DOSJETOS DEOEDO



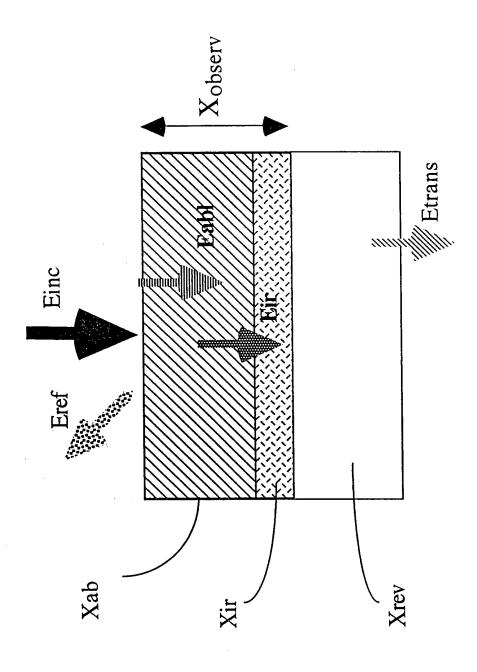


Fig. 10a

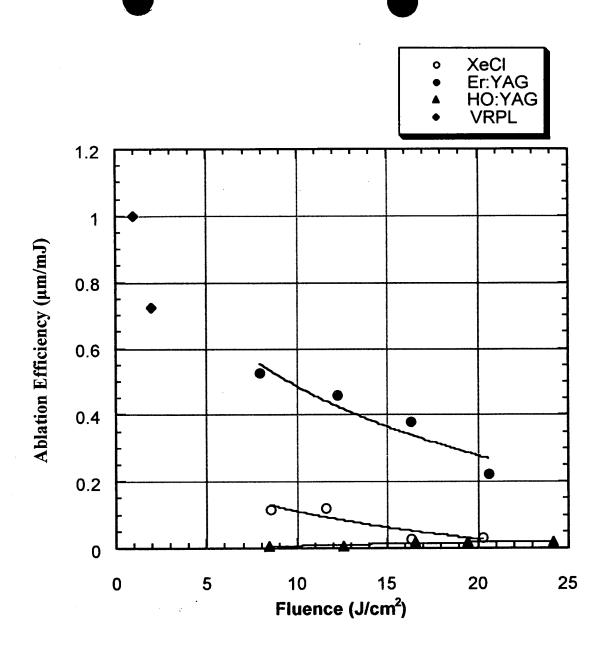
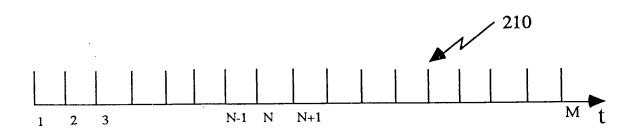
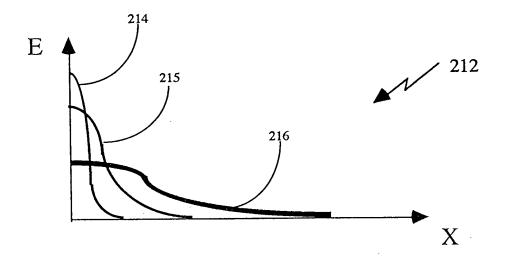


Figure 10b






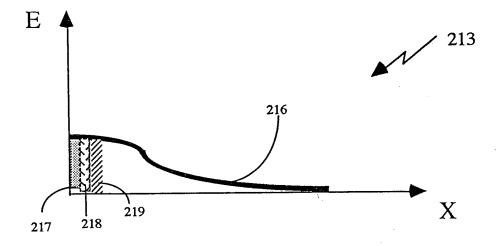


Fig. 11

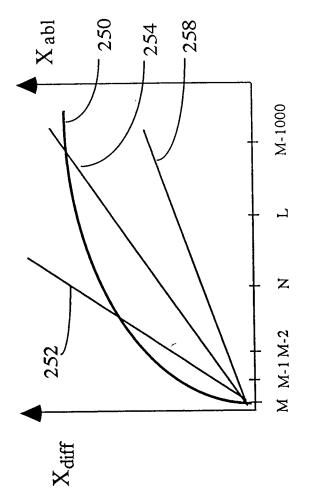

Pulse Number

FIG. 12

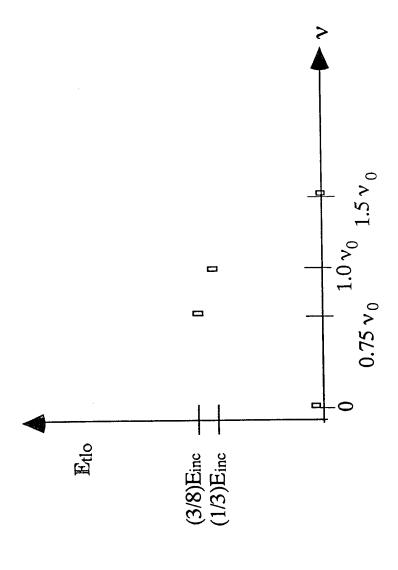


FIG. 13

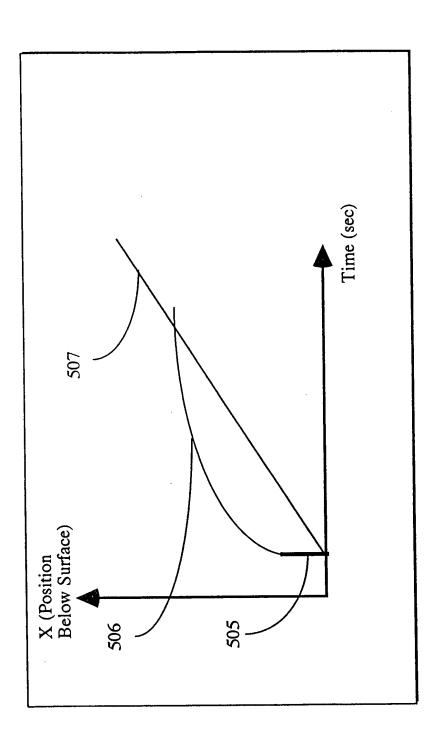


Fig. 14

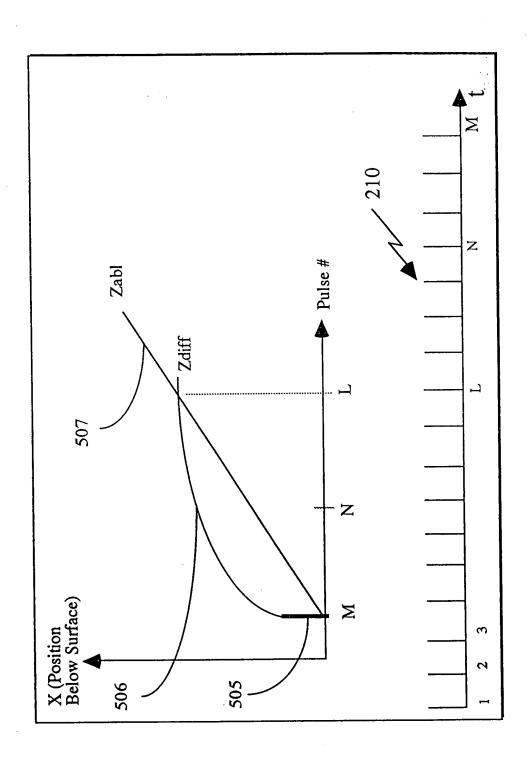


Fig. 15

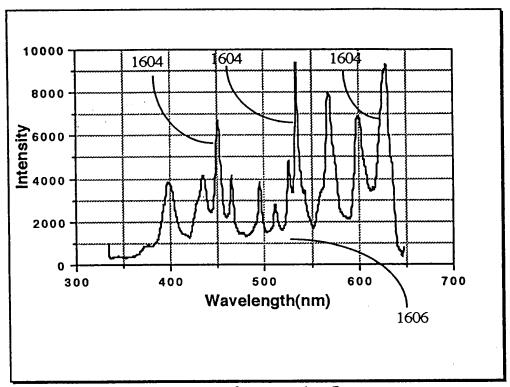


Fig. 16a

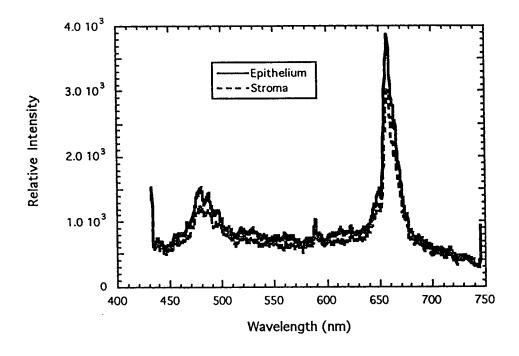


Fig. 16b

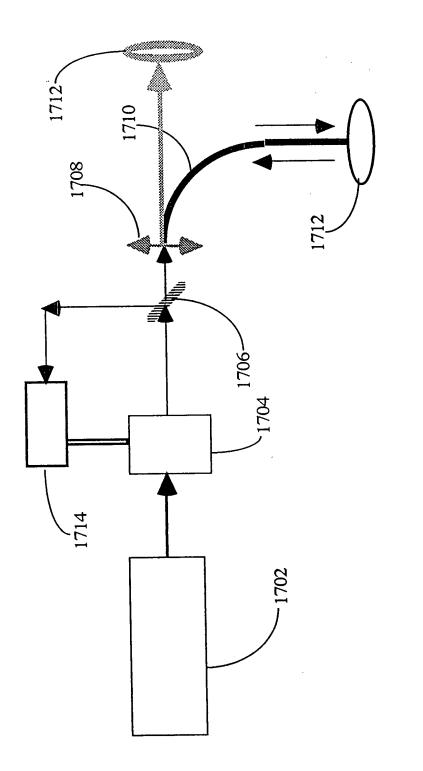


Fig. 17

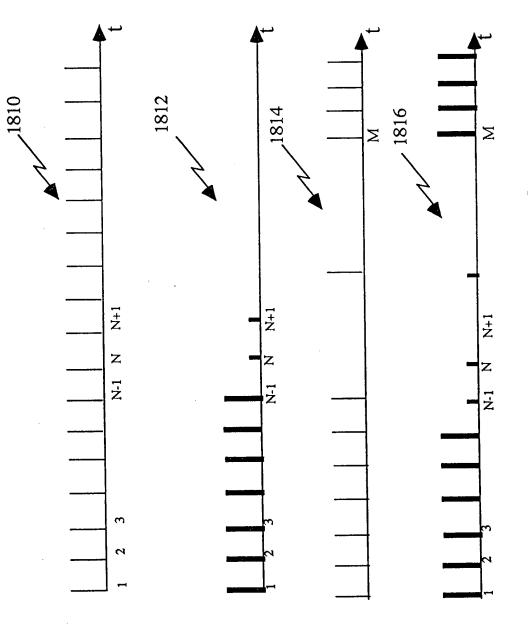


Fig. 18